




# Transfer Board

 Caution: Read Instructions before operating device.

 Caution: Use caution when using device to avoid pinching or trapping fingers.

## Care and Cleaning

1. Hand wipe with mild detergent and water using damp cloth. Dry thoroughly.

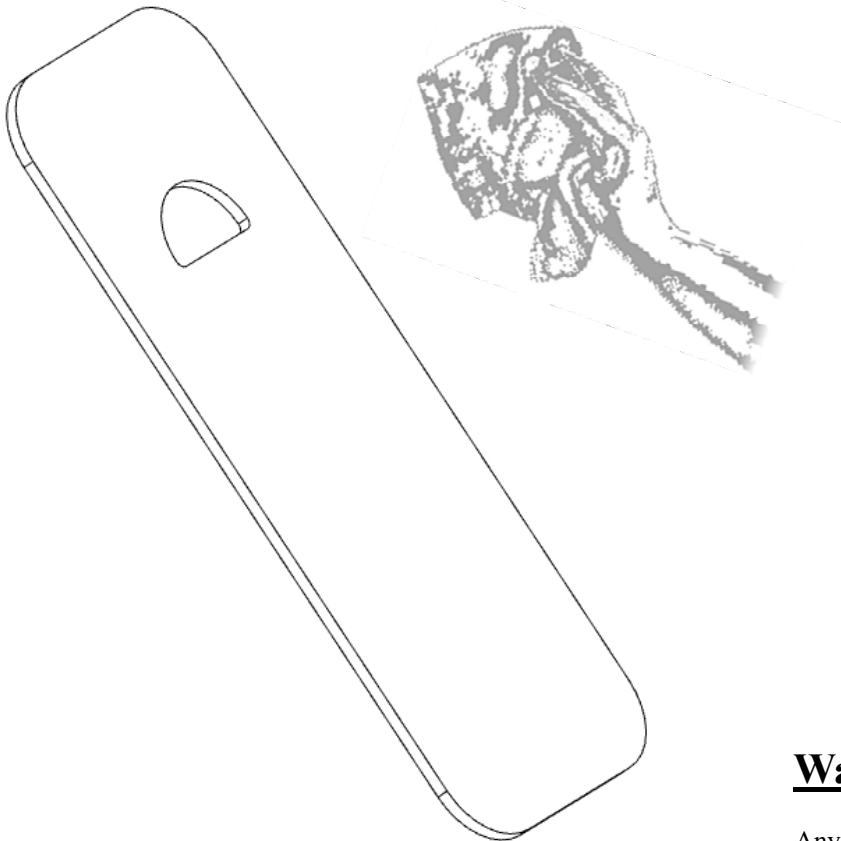

## Warranty

Any product found to be defective due to the material or workmanship within one year will be replaced under our return policy following product evaluation by Therafin Corporation. This replacement warranty does not include misuse or neglect of the product.



 Therafin Corporation  
9450 W Laraway Road  
Frankfort, IL 60432 USA  
800-843-7234